


MS 2600 NG – PATCH :

MS 2600 NG

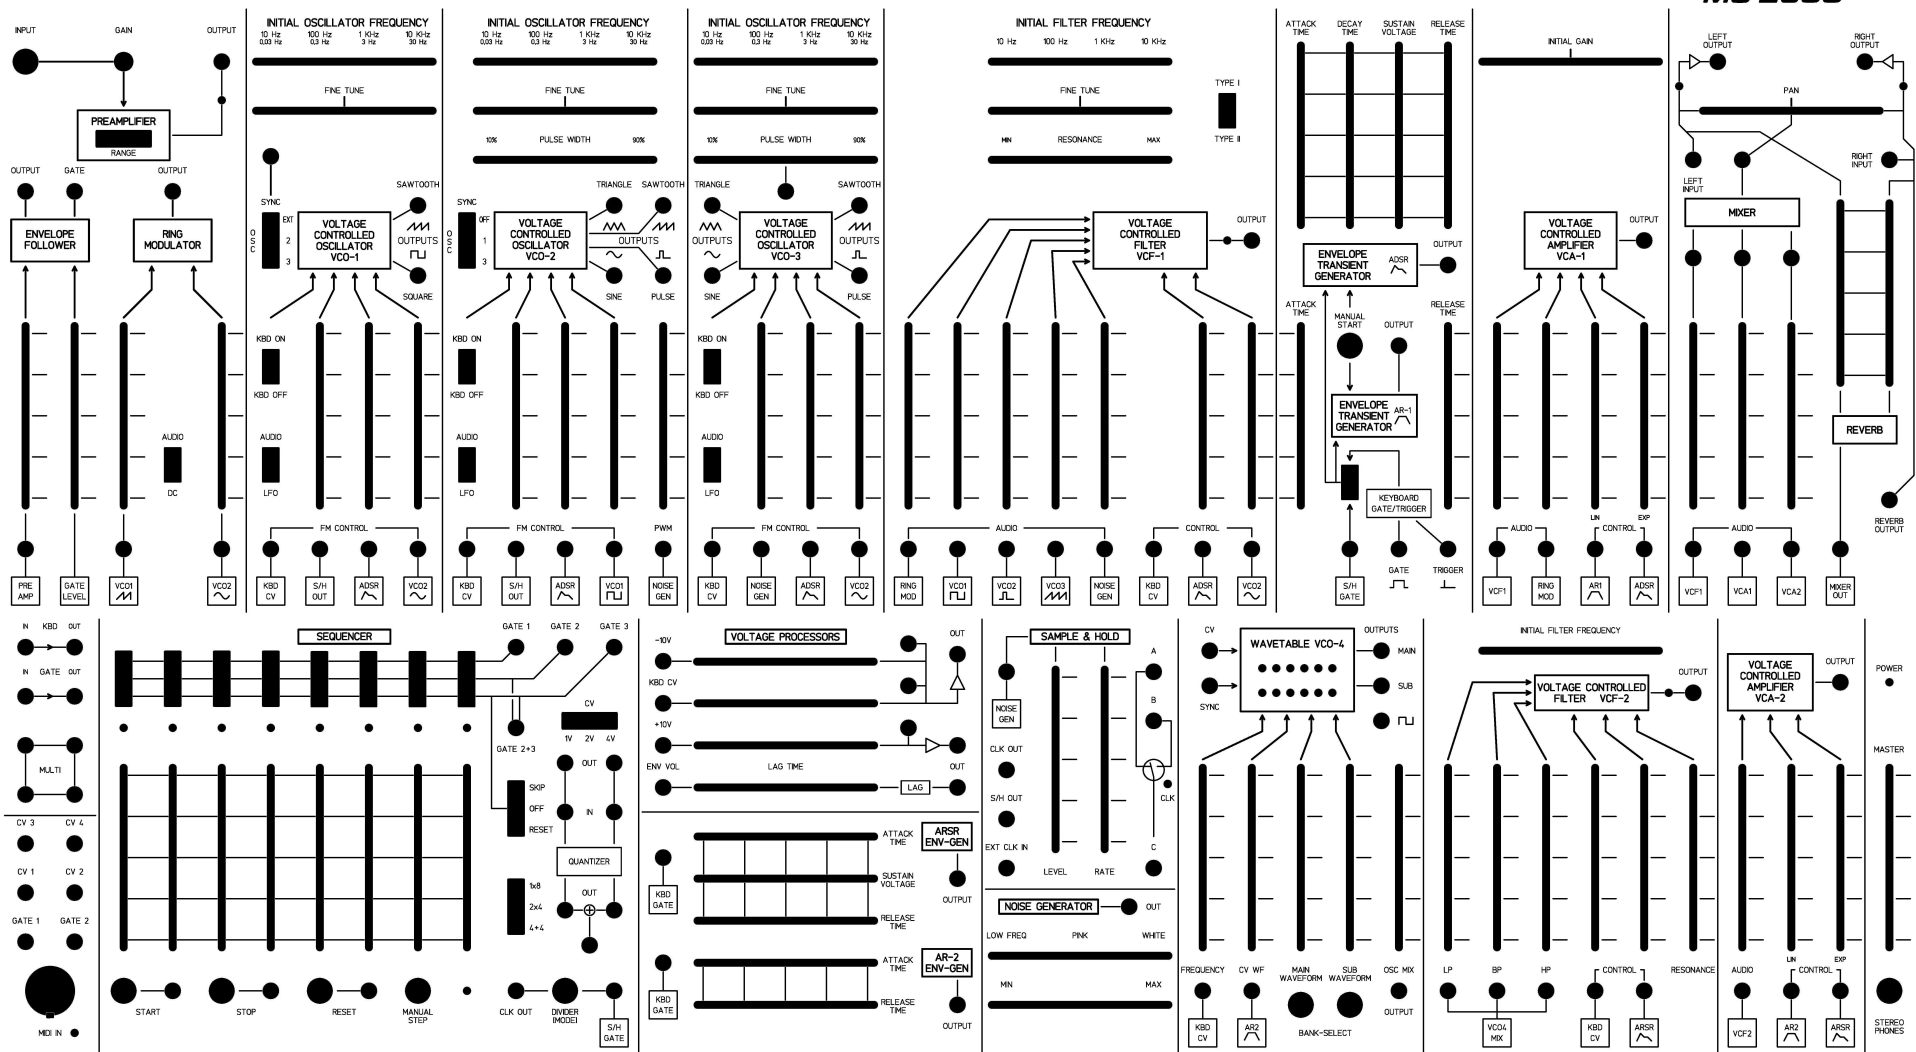

SEQ-SETUP:

- | | | | |
|--|--------------------------------------|----------------------------------|------------------------------|
| <input type="checkbox"/> UP | <input type="checkbox"/> UP&DN | <input type="checkbox"/> 16 RND | <input type="checkbox"/> RND |
| <input type="checkbox"/> Single | <input type="checkbox"/> Repeat | <input type="checkbox"/> WF-Gen. | |
| <input type="checkbox"/> OUT A,B | <input type="checkbox"/> OUT A+B | | |
| Quantizer <input type="checkbox"/> Chromatisch | <input type="checkbox"/> Individuell | | |
| Quantizer <input type="checkbox"/> CLK | <input type="checkbox"/> FREE | | |
| Teiler <input type="checkbox"/> | | | |

VCO4-SETUP:

- MAIN: OSC-Grundton:
- KBD CV FREQ. FINE CV chrom. CV linear CV WF LFO
- SUB: OSC-Grundton:
- KBD CV FREQ. FINE CV chrom. CV linear CV WF LFO